

Crystal Digital PCR® Assay

Information Sheet

For Research Use Only. Not for use in diagnostic procedures.

Product Name

AAV Crystal Digital PCR® Assay (R53002)

Description

Detected AAV Targets

Targets	Sample Type	Detection Channels	Multiplex
AAV Vector Regulatory Elements	DNA	Blue/Teal/Green/Yellow/Red/ Infra-Red/Long-Shift	Up to 7-plex

The AAV Crystal Digital PCR® Assay is a 10X multiplexed assay designed to detect and quantify key regulatory elements of adeno-associated virus (AAV) vectors, enabling vector integrity assessment using the Ruby Chip. Its flexible mix-and-match feature allows customization across diverse cell and gene therapy workflows.

AAV vectors are essential for efficient gene delivery, stable transgene expression, and safety in gene therapy applications. Their manufacturing and purification require stringent quality control to ensure safe and consistent dosing in both clinical trials and patient treatments, as mandated by regulatory agencies.

This assay delivers a robust and precise solution for vector copy number (VCN) quantification, contamination detection, and viral genome integrity assessment—critical parameters for ensuring batch-to-batch consistency in AAV vector production. An indispensable tool for biopharma manufacturers and researchers, it streamlines QC workflows while supporting regulatory compliance in gene therapy development.

Assay Configuration

The AAV Crystal Digital PCR® Assay configuration is modular, which allows to build an assay according to targets of interest. Select one target per color to combined within a panel for 1-plex up to a 7-plex assay*.

Blue	Teal	Green	Yellow	Red	Infra-Red	Long-Shift
CMV promoter	GFP / YFP / CFP	ITR2	bGH	WPRES	Kanamycin Resistance 3'	Kanamycin Resistance 5'
hSyn	-	-	SV40 polyA	CMV enhancer	NeoKanamycin Resistance 3'	NeoKanamycin Resistance 5'

*More AAV targets available soon.

Components

AAV Crystal Digital PCR® Assay comprises two types of reagents:

1. A pool of the target specific primers and Crystal Flex Probes. One separate tube is provided per AAV target.
2. Positive Control. Please refer to the lot specific Certificate of Conformity for characterized concentration, available upon request to the Stilla Technologies Technical Support team (support@stilla.fr).

Component Name	Reference	Concentration	Description
AAV cdPCR Assay [Target]	R53002.Target	40X	Contains the pool of specific primers and Crystal Flex Probes for each corresponding AAV target.
AAV Positive Control	R53002.PC0	10X	Contains synthetic target DNA

Thermocycling Programs

On the Nio® Digital PCR:

Step		Ramp rate
Step 1	Partition for Ruby Chip	-
Step 2	Temperature 95°C for 180 seconds	1°C/sec
Step 3	Begin Loop for 60 Iterations	-
Step 3.1	Temperature 95°C for 15 seconds	2°C/sec
Step 3.2	Temperature 60°C for 30 seconds	2°C/sec
Step 4	Temperature 58°C for 300 seconds	1°C/sec
Step 5	Release for Ruby Chip	-

Image Acquisition

Download the dedicated scanning file from the Technical Resources section of the Stilla Technologies website:

- NioProtocol_7C-60X-60°C-30s_v2.nioprotocol (Nio Digital PCR)
- NioAssay_7C_AAV_v3.nioassay (Nio Digital PCR)

Image Analysis

The following files are embedded in the dedicated scanning files listed above:

- CompensationMatrix_Nio_AAV_v2.ncm

Consumables Required but Not Provided

- Ruby Chip (C16011)
- naica® PCR MIX 10X (R10106)
- Depending on the selected AAV targets:
 - Crystal Universal Reporters 3 (R41401 200 reactions, R41402 1000 reactions)
 - Crystal Universal Reporters 7 (R42401 200 reactions, R42402 1000 reactions)
- Nuclease-free water

Instruction for PCR Mix Preparation

Specific instructions for preparing the PCR mix are given below. Depending on the selected AAV targets, two PCR mix preparation tables are possible. Stilla recommends preparing a pool for at least 10 chambers.

For AAV targets using **Blue**, **Green**, and/or **Red**:

Reagent Name		Initial Concentration	Final Concentration	Volume per reaction (μL)
naica® PCR MIX Buffer A	●	10x	1x	0.60
naica® PCR MIX Buffer B	●	100%	4%	0.24
Crystal Digital PCR® Assay	●	Add from 1 to 3 target assays		
<i>Target blue (optional)</i>		40x	1x	0.15
<i>Target green (optional)</i>		40x	1x	0.15
<i>Target red (optional)</i>		40x	1x	0.15
Crystal Universal Reporter Tube A	●	40x	1x	0.15
Nuclease-free water		NA	NA	Variable
Template DNA, or		NA	NA	Variable
<i>Positive Control Target blue</i>	○	10x	1x	0.60
<i>Positive Control Target green</i>	○	10x	1x	0.60
<i>Positive Control Target red</i>	○	10x	1x	0.60
<i>Total reaction volume (μL)</i>				<i>6.0</i>

Note for Resistance Gene targets: their synthetic DNA Positive Control corresponds to the full sequence (including the 5' and 3' ends) of the resistance gene. Therefore, if both targets (5' and 3') are included in a given assay configuration, the Positive Control should be included only once to obtain the expected quantification.

For AAV targets using **Blue**, **Teal**, **Green**, **Yellow**, **Red**, **Infra-Red**, and/or **Long-Shift**:

Reagent Name		Initial Concentration	Final Concentration	Volume per reaction (µL)
naica® PCR MIX Buffer A	●	10x	1x	0.60
naica® PCR MIX Buffer B	●	100%	4%	0.24
Crystal Digital PCR® Assay	●	Add from 1 to 7 target assays		
<i>Target blue (optional)</i>		40x	1x	0.15
<i>Target teal (optional)</i>		40x	1x	0.15
<i>Target green (optional)</i>		40x	1x	0.15
<i>Target yellow (optional)</i>		40x	1x	0.15
<i>Target red (optional)</i>		40x	1x	0.15
<i>Target infra-red (optional)</i>		40x	1x	0.15
<i>Target long-shift (optional)</i>		40x	1x	0.15
Crystal Universal Reporter Tube A*	●	40x	1x	0.15
Crystal Universal Reporter Tube B	●	40x	1x	0.15
Nuclease-free water		NA	NA	Variable
Template DNA, or		NA	NA	Variable
<i>Positive Control Target blue</i>	○	10x	1x	0.60
<i>Positive Control Target teal</i>	○	10x	1x	0.60
<i>Positive Control Target green</i>	○	10x	1x	0.60
<i>Positive Control Target yellow</i>	○	10x	1x	0.60
<i>Positive Control Target red</i>	○	10x	1x	0.60
<i>Positive Control Target infra-red</i>	○	10x	1x	0.60
<i>Positive Control Target long-shift</i>	○	10x	1x	0.60
Total reaction volume (µL)				6.0

*Crystal Universal Reporter Tube A must always be included in the reaction mix, even if none of the targets are detected in blue, green, or red for given assay configuration.

Note for Resistance Gene targets: their synthetic DNA Positive Control corresponds to the full sequence (including the 5' and 3' ends) of the resistance gene. Therefore, if both targets (5' and 3') are included in a given assay configuration, the Positive Control should be included only once to obtain the expected quantification.

Representative Data and Instructions for Analysis

Set thresholds for separating positive and negative populations on the 1D plots. To optimize the analysis, the thresholds should be set at approximately equal distance from the positive and negative clusters. Wet lab testing was carried out using synthetic single strand DNA as positive control. Examples of results obtained on the Nio+ configuration are given below.

For integrity analysis, contact our Technical Support team (support@stilla.fr) to obtain a personalized **Analysis Configuration File** and **Excel Analysis Workbook** corresponding to the assay level of plex and targets selected.

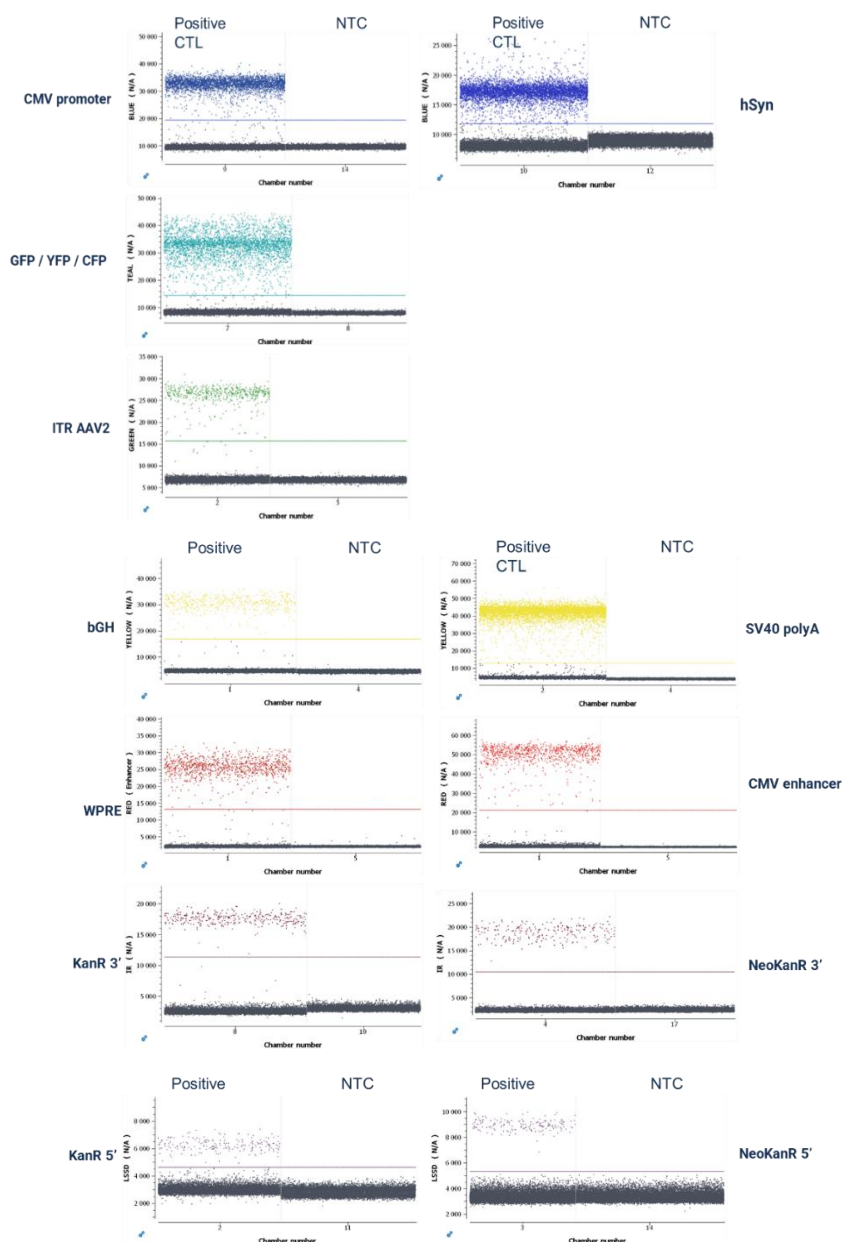


Figure 1: 1D plots obtained with each of the targets of the AAV Crystal Digital PCR® Assay during wet lab testing on Nio Digital PCR.

These data have been obtained using simplex assays. When using multiplex assays (combination of several target assays) separability scores may be different. Stilla recommends validating the assay in multiplex with final samples.



Stilla Technologies
F-94800 Villejuif, FRANCE

Registered names and trademarks used in this document, even when not specifically marked, are not to be considered unprotected by law.